



Reprocessing Guide for LM™ dental instruments

LM

feel the
difference



This guide includes recommendations on how to reprocess LM™ dental instruments

LM-Dental™ recommends the use of validated cleaning, disinfection and/or sterilization procedures described in this processing instruction according to standard ISO 17664. This guide is applicable for LM™ hand instruments, LM™ care and handling products, LM™ extraction instruments, LM™ scaler tips and polisher nozzles as well as LM™ accessories that needs to be reprocessed before use.



CONTENT

1. INTRODUCTION.....	3
1.1 The processing steps provided herein.....	3
1.2 LM-Servo™ system.....	3
1.3 Disclaimer.....	3
2. WARNINGS.....	4
3. PRECAUTIONS	4
3.1 General.....	4
3.2 Material resistance.....	4
4. REPROCESSING INSTRUCTIONS	5
4.1 General.....	6
4.2 Processing instructions.....	7
ANNEX 1: LIST OF PRODUCTS COVERED BY THIS GUIDE	

1. INTRODUCTION






1.1 The processing steps provided herein

Apply to the products indicated for dental periodontics, diagnostics, restoration, extraction, endodontics, implant surgery and orthodontics before use and/or reuse. Are intended to be performed only in a dental or hospital environment, by dentists, dental hygienists, or qualified users, following good dental practices.

The processing of products applies to the following situations:

- All LM™'s products are supplied in a non-sterile condition. Processing prior to first use is required.
- All products mentioned in this guide are reusable products. Processing is required after each use prior to reuse.

The table below summarizes the various existing situations and types of processing actions that are applicable:

Symbol on package or product	Device used to perform processing	Processing step
	Ultrasonic bath	Pre-cleaning
	Washer-Disinfector	Cleaning and disinfection
	Steam sterilizer	Sterilization

This guide is applicable to the products listed in [Annex 1: List of products covered by this guide](#).



Note! Regularly service the maintenance devices and follow all instructions in this guide.

Note! Pay special attention to correct dosage and exposure of disinfectants and cleaning agents.

Note! LM™ does not recommend manual cleaning - washer-disinfector is the only method that is validated.

1.2 LM-Servo™ system



Note! Use LM™'s instrument cassettes to protect the instruments and avoid sharp injuries.

LM-Servo™ system is an instrument handling and maintenance concept for dental professionals. It organizes and rationalizes the handling of dental instruments and accessories during the reprocessing procedures and maintenance. LM-Servo™ system facilitates a good hygiene control and saves your time by minimizing the handling of the individual items. The system prolongs the life span of instruments and protects the dental personnel. More information on system at www.lm-dental.com/products/care-and-handling

1.3 Disclaimer

The instructions for processing products before first use/reuse herein have been validated by LM-Instruments Oy. Users are solely responsible for any deviation from these instructions, and/or the use of alternative methods for processing. LM-Instruments Oy accepts no liability for damage, injury, or any legal responsibility incurred directly or indirectly by the user due to a deviation from the guide set forth below. The user shall observe safe and lawful practices including, but not limited to, those outlined in this document.

2. WARNINGS



- Reusing these products without sterilization increases the risk of cross-contamination.
- Reusable products must be cleaned and sterilized prior to first use.
- The recommended maximum temperature of the steam sterilizer for reprocessing LM™ products is 134°C-137°C (273°F-278°F).
- Liquids containing chlorine, phenol or amines are not permitted to use for reprocessing LM™ products.
- A steel brush or any other sharp or abrasive tools are forbidden to be used for instrument cleaning as they will damage the metal blades and the silicone handles, thereby reduce the lifetime of the product.
- Do not use any abrasive tools for removing residue from LM Dark Diamond™ and LM Sharp Diamond™ instruments as they will damage the special coating and thus reduce the lifetime of the product.
- During the sterilization process, the residue may bake into the instrument handle resulting in discolorations.
- Do not soak any of LM™ products in lubricants.
- LM DTS™ product and the tagging might be damaged if it is heavily exposed to mineral oils.
- We don't recommend hot air sterilization but if anyway proceeding with this method note that the package of your product is marked with maximum sterilization temp of 180°C.
- Do not sterilize any of LM™ products in autoclaves that have oil residues in the chamber.

3. PRECAUTIONS



3.1 General

- Dispose of all sharp and contaminated products in accordance with accepted local regulations.
- Always wear protective clothes for your safety (gloves, eye protection wear, and mask).
- Do not use labels or identification markers directly on the product.
- Only use properly maintained processing equipment and materials approved by national laws and regulations. The reprocessing equipment should be used according to the manufacturer's instructions (including calibration, cleaning, loading weight, shelf life, operating, time and functional testing).
- Only use a detergent solution with disinfecting action approved for its efficacy (VAH/DGHM listing, CE marking, FDA approval) and in accordance with the IFU of its manufacturer.
- Detergent should be aldehyde-free (to avoid blood and exposure time impurity fixation).
- Always follow the instructions and concentrations provided by the manufacturer of the cleaning/disinfecting agent.
- Remove residue (especially filling materials residue) from instruments blades and handles while still soft.

For LM™ hand instruments, LM™ extraction instruments, LM™ scaler tips, and LM™ polisher nozzles

Inspect the products before reuse and discard them in case of one of the following defects occurs:

- Breakage;
- Loss of color coding or marking;
- Bent instrument;
- Damaged threads on scaler tips and polisher nozzles;
- Damaged cutting surfaces;
- Dull cutting blades;
- Missing UDI code or product marking;
- Corrosion.

3.2 Material resistance

Incorrect use of cleaning and disinfecting agents can damage the products. Consult the instructions for use provided by the legal manufacturer of the cleaning/disinfection agent and check compatibility with the material of the products.

A non-exhaustive list of situations to avoid:

- NiTi products should not be fully immersed in NaOCl solution concentrate. Only the operative part, which is in contact with the patient, should be immersed. The NaOCl solution concentration shall not exceed 5%.
- Do not use solutions containing phenol or any products which are not compatible with the products.
- Excessive concentrations or immersion / exposure times may cause corrosion or other defects in the products.
- It is recommended to use an alkaline / exposure detergent with surfactants, with grease removal, disinfection (against bacteria/fungi) and corrosion inhibition properties.

4. REPROCESSING INSTRUCTIONS



4.1 General

Instruction for processing prior to use/reuse

Type of product family	Condition	Instruction
LM™ diagnostic hand instruments LM™ restorative hand instruments LM™ endodontic hand instruments LM™ orthodontic hand instruments LM™ periodontal hand instruments LM™ implant surgery hand instruments LM Dark Diamond™ (DD) instruments	Processing before first use	Steps 5 to 9
	Processing before reuse	Steps 1 to 9
LM Sharp Diamond™ (SD) instruments	Processing before first use	Steps 5 to 9
	Processing before reuse	Steps 1 to 9
LM™ ultrasonic tips LM™ polisher nozzles LM-ErgoGrip™	Processing before first use	Steps 5 to 9
	Processing before reuse	Steps 1 to 9
LM™ accessories and care/handling products	Processing before first use	Steps 5 to 9
	Processing before reuse	Steps 1 to 9

4. REPROCESSING INSTRUCTIONS



4.2 Processing instructions

Processing instructions for **LM™ hand instruments**, **LM™ care & handling products**, **LM™ extraction instruments**, **LM™ scaler tips** & **polisher nozzles** and **LM™ accessories**.




Operation	Operating mode	Precautions in addition to section 3. PRECAUTIONS
1. Initial treatment at the point of use	General instructions: <ul style="list-style-type: none"> - Rinse the lumen line for one minute with cold tap water (minimum drinking quality 20± 2°C) if the instrument has a lumen. - Do not leave dirty instruments to dry if not able to clean within 4 hours; soak all products in a pre-cleaning solution according to the manufacturer's instructions (aldehyde-free and intended for pre-cleaning by the manufacturer. (A washing medium at 0,5% concentration including (according to Regulation (EC) No 648/2004) less than 5%: anionic/non-ionic surfactants and with pH 10, was utilized for a minimum of 10 min. in deionized water at temp 30°C for Validation procedure). Where applicable use a tray made from high-density polyethylene or stainless steel. 	<ul style="list-style-type: none"> - The pre-cleaning solution should be changed regularly i.e. when it becomes soiled, or when efficacy is diminished due to exposure to microbial loads. - Only use clean soft brushes designed for this purpose. Do not use metal brushes. - Don't mix instrument with different steel materials like LM Sharp Diamond™ and standard instruments.
2. Containment and transport	Safely transport to reprocessing area. It is recommended to reprocess the medical devices as soon as possible after use.	—
3. Preparation before cleaning	For visible impurities observed on products, or when needed, mechanical pre-cleaning with a soft brush made from either nylon, polypropylene or acrylic is recommended. Manually brush the product until visible impurities are removed.	—
4. Pre-cleaning & Rinsing (Optional)	Ultrasonic bath <ul style="list-style-type: none"> - Immerse the instruments in the detergent solution with cleaning properties according to the manufacturer's instructions (a washing medium at 0,5% concentration including (according to Regulation (EC) No 648/2004) less than 5%: anionic/non-ionic surfactants and with pH 10. Assisted by an ultrasonic device for at least 15 minutes in deionized water at temp 30°C. - For visible impurities observed on products: manually brush the instruments for one minute until visible impurities are removed (use a soft brush made from either nylon, polypropylene or acrylic). - Rinse thoroughly (at least one minute) under running cold deionized water. 	<ul style="list-style-type: none"> - Always place the products in a cassette, support or container to avoid any contact between products. - Don't mix instrument with different steel materials like LM Sharp Diamond™ and standard instruments
5. Automated cleaning with washer-disinfector Cleaning Disinfection Drying	<ul style="list-style-type: none"> - Use a detergent solution with cleaning properties (a washing medium at 0,5% concentration including (according to Regulation (EC) No 648/2004) less than 5%: anionic/non-ionic surfactants and with pH 10, was utilized for a minimum of 10 min. in deionized water at temp 55°C for Validation procedure). - Place the products in a cassette, support or container to avoid any contact between products. LM-Servo™, LM-Servo™ E, and LM-ServoMax™ system are recommended to reprocess LM™ devices. And if the washer-disinfector has special lumen adapters*) use that for products with lumen. - Place the products in a washer disinfector in accordance with EN ISO 15883-1+-2 with thermal program (temperature 90-95°C (194-203°F) and perform the defined cycle A0≥3000. 	<ul style="list-style-type: none"> - Pay particular attention to cutting edges and sharp edges, both to avoid injury and damage to the products. - Follow carefully the instruction provided by the disinfection solution manufacturer.

*) Here you can use special rinsing adapters from washer-disinfector manufacturers special designed for LM™ ultrasonic scaler tips:

- Miele
- Melag
- IC Medical

4. REPROCESSING INSTRUCTIONS

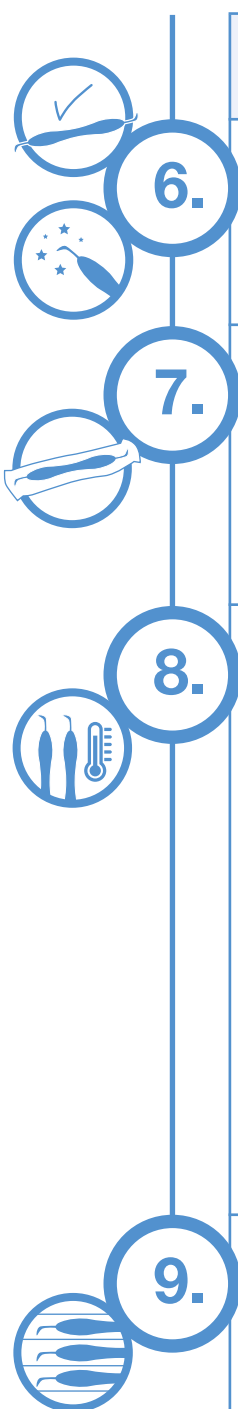

Operation	Operating mode	Precautions in addition to section 3. PRECAUTIONS
Maintenance, inspection & testing	<ul style="list-style-type: none"> - Inspect the product functionality (check the sharpness of cutting parts if applicable). - Visually inspect the product with the naked eye under appropriate lighting (min. 500 lux) and discard if there are any defects (e.g. cracks, deformations, breakage, corrosion, loss of color coding, or marking). - Dirty products should be processed again. 	—
Packaging	<ul style="list-style-type: none"> - Place the products in a cassette, support or container to avoid any contact between products. - Pack the products in "Sterilization pouches" (double-packaged using paper-plastic pouches for steam sterilization). - For sharp products that are not contained within a box, silicone tubes should be placed around the products to prevent piercing of the packaging. - Seal the pouches according to the pouch manufacturer's recommendations. 	<ul style="list-style-type: none"> - Ensure that the pouches are suitable for steam sterilization (141°C, 286°F) and validated and manufactured as per ISO 11607 and EN 868-5. - If a thermo-sealer is used, the process must be validated and the thermosealer must be calibrated and qualified.
Sterilization	<ul style="list-style-type: none"> - Place the pouches in the steam sterilizer according to the manufacturer's recommendations. - Use one of the following sterilization cycles with the Pre-vacuum air removal steam sterilizer (saturated steam and compliant with EN 13060 (class B, small sterilizer) and EN 285 (full-size sterilizer)): <ul style="list-style-type: none"> • 132°C-135°C (270°F-275°F), 4 minutes; • 134°C-137°C (273°F-278°F), 3 minutes; <p>We recommend steam sterilization at 134°C / 273.2°F for 3 minutes for deactivating potential prions.</p> <ul style="list-style-type: none"> - Visually inspect the product with the naked eye under appropriate lighting (min. 500 lux) for packaging integrity, humidity, color change of packaging, positive physical-chemical indicators and conformity of actual cycle parameters with the reference cycle parameters. - If visible signs of moisture are present (damp spots on sterile packaging, pooled water in the load) at the end of the sterilization cycle, repackage and re-sterilize using a longer drying time. - Store traceability records. 	<ul style="list-style-type: none"> - Use a validated sterilization procedure according to ISO 17665 with a minimum drying time of 20-minutes. - Special attention should be paid to the packaging integrity if the 134°C (273.2°F) 3 minutes sterilization cycle is used. - Check the pouch's validity period indicated by the manufacturer to determine the shelf life. - The owner is responsible for complying with the sterilizer's maintenance procedure, which should be performed in accordance with the requirements on sterilizing medical devices (examples: planning for maintenance, qualification, acceptance criteria condensate and water as per EN 285, annex 2).
Storage	<ul style="list-style-type: none"> - Keep sterilized packaged products in a clean environment, away from moisture and direct sunlight. Store at ambient temperature (typically 15-25°C (59-77°F)). - In case of damage to the pouch, a complete new processing cycle should be performed. - Check the packaging and the medical devices before using them (packaging integrity, humidity, and expiry date). 	<ul style="list-style-type: none"> - After sterilization, the product should be handled with care to keep the packaging intact (sterile barrier). Sterility cannot be guaranteed if the packaging is open, damaged, or wet.
Additional information	The processing of medical devices should be done with validated processes.	
Manufacturer contact	<div> <div>LM-Instruments Oy Norrbyn rantatie 8 21600 Parainen Finland</div> <div> info@lm-dental.com Tel +358 2 454 6400 www.lm-dental.com </div> </div>	

The processing of medical devices should be done with validated processes.

The recommended instructions provided above have been validated by the manufacturer of the medical device as being capable of preparing a medical device for reuse. It remains the responsibility of the processor to ensure that the processing, as performed using equipment, materials, and personnel in the processing facility, achieves the desired results. This requires verification and/or validation and routine monitoring of the process.

ANNEX 1: LIST OF PRODUCTS COVERED BY THIS GUIDE



Type of product family	Product code	Delivered in sterile condition	
LM™ diagnostic hand instruments	For a complete product code list ask your LM™ distributor	No	CE
LM™ restorative hand instruments	For a complete product code list ask your LM™ distributor	No	CE
LM™ endodontic hand instruments	For a complete product code list ask your LM™ distributor	No	CE
LM™ orthodontic hand instruments	For a complete product code list ask your LM™ distributor	No	CE
LM™ periodontal hand instruments	For a complete product code list ask your LM™ distributor	No	CE
LM™ extraction instruments	For a complete product code list ask your LM™ distributor	No	CE
LM™ implant surgery hand instruments	For a complete product code list ask your LM™ distributor	No	CE
LM™ ultrasonic tips LM™ polisher nozzles	For a complete product code list ask your LM™ distributor	No	CE ₀₅₃₇
LM™ accessories & care/ handling devices	For a complete product code list ask your LM™ distributor	No	CE

Exclusively distributed by Curion

curion.ca | **EN: 1.800.667.8811** | **FR: 1.800.211.1200**



LMDental™

 LM-Instruments Oy | Norrbyn rantatie 8 | FI-21600 Parainen, Finland |

Tel. +358 2 4546 400 | info@lm-dental.com | www.lm-dental.com

